




Customer: Box State
Customer Sample ID: 9/24 Second Pass
Laboratory Number: 19I0423-01

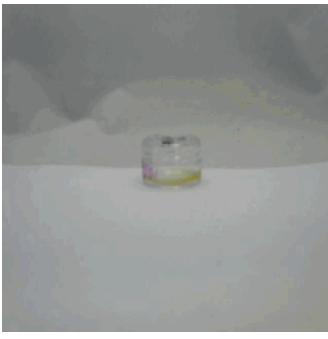


Cannabinoid Profile

Extraction Technician: DF
Analytical Chemist: GB

Extraction Date(s)	Analysis Date(s)
9/25/2019	9/25/2019

Cannabinoids (HPLC)		Results	
	LOD (mg/g)	%	mg/g
Cannabidivarin (CBDV)		0.73	7.28
Cannabidiolic Acid (CBD-A)	<0.20		
Cannabigerolic Acid (CBG-A)	<0.20		
Cannabigerol (CBG)		1.50	15.0
Cannabidiol (CBD)		79.80	798
Tetrahydrocannabivarin (THCV)	<0.20		
Cannabinol (CBN)		0.22	2.17
delta 9-Tetrahydrocannabinol (THC)		3.17	31.7
delta 8-Tetrahydrocannabidol		0.13	1.32
Cannabichromene (CBC)		0.46	4.60
delta-9-Tetrahydrocannabinolic Acid (THC-A)	<0.20		
Cannabinoids Total		%	mg/g
Max Active THC		3.17	31.70
Max Active CBD		79.80	798.00
T.Active Cannabinoids		85.1	851
Total Cannabinoids		86	860
Ratios			
25.19:1 CBD to THC		0.04:1 THC to CBD	

Cannabinoid (mg/g)

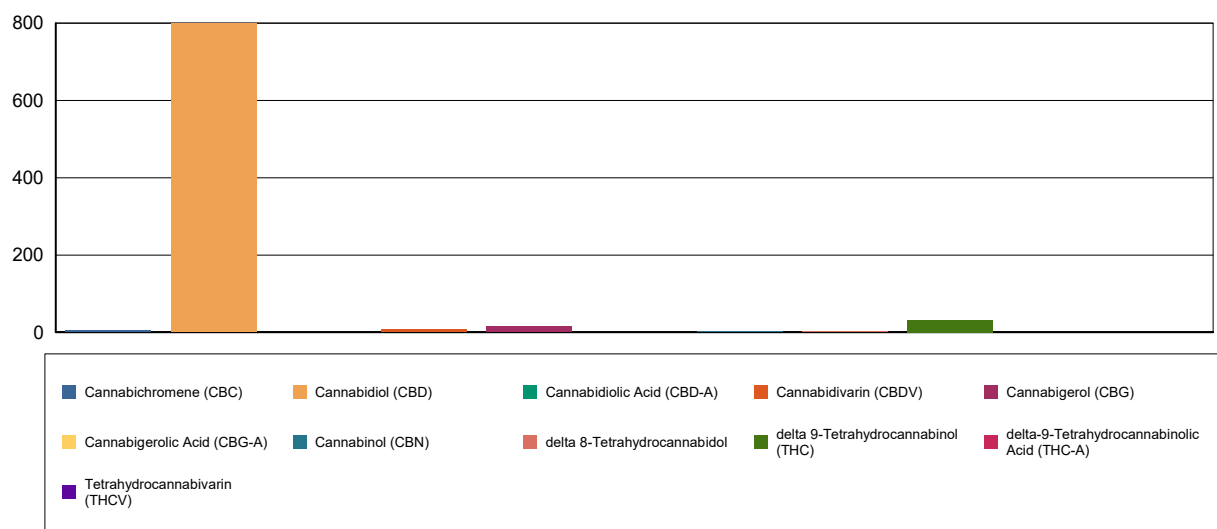

Altitude Consulting, LLC utilizes NIST traceable Reference Standards and Certified Reference Material to calibrate analytical instruments along with proven analytical methods. The methods are applied in the most ethical manner following good laboratory practice guidelines. The results of this report are based solely on the sample submitted and cannot be reproduced.



Customer: Box State
Customer Sample ID: 10/8 Batch #1
Laboratory Number: 19J0175-03



Residual Solvents Profile

Extraction Technician: RH
 Analytical Chemist: MF

Extraction Date(s)	Analysis Date(s)
10/9/2019	10/9/2019

Residual Solvents	Results	Calibration Range
	ug/g	
Propane	<96.5	100 - 2000
Isobutane	<96.5	100 - 2000
Methanol	<96.5	100 - 2000
Butane	<96.5	100 - 2000
Isopropanol	<96.5	100 - 2000
Ethanol	<96.5	100 - 2000
2-Methyl Butane	<96.5	100 - 2000
Acetonitrile	<96.5	100 - 2000
Acetone	<96.5	100 - 2000
n-Pentane	<96.5	100 - 2000
n-Hexane	<48.3	50 - 2000
Tetrahydrofuran	<96.5	100 - 2000
Benzene	<0.965	1.0 - 50
n-Heptane	<96.5	100 - 2000
Toluene	<96.5	100 - 2000
Ethylbenzene	<96.5	100 - 2000
m+p Xylene	<96.5	100 - 2000
o-Xylene	<96.5	100 - 2000
Total Xylenes	<96.5	100 - 2000
1,2,3-Trimethylbenzene	<96.5	100 - 2000

Altitude Consulting, LLC utilizes NIST traceable Reference Standards and Certified Reference Material to calibrate analytical instruments along with proven analytical methods . The methods are applied in the most ethical manner following good laboratory practice guidelines. The results of this report are based solely on the sample submitted and cannot be reproduced.



Customer:


Customer Sample ID:

Laboratory Number:

Box State

Batch #1

19J0295-01

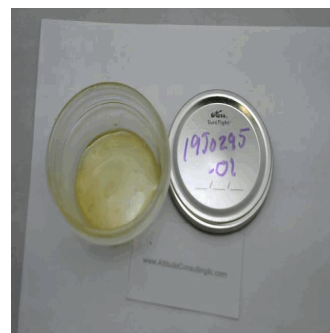

Metals Profile

Extraction Technician: MF

Analytical Chemist: MF

Extraction
Date(s)

10/15/2019

Analysis
Date(s)

10/25/2019

Metals (ICP/MS)	Method Code	Results	Units
Arsenic	ICPMS.1	<20.0	ppb
Cadmium	ICPMS.1	<10.0	ppb
Lead	ICPMS.1	<5.00	ppb
Mercury	ICPMS.1	<5.00	ppb

Limits for metals vary greatly depending on usage of the sample. Altitude Consulting recommends researching federal and state regulatory limits.